

Quick Start Guide



IMPORTANT: COMPLETE ALL STEPS BELOW TO ENSURE INTENSITY LEVEL RESET TO "0" DOES NOT INITIATE.


Step 1. Insert 3 AAA Batteries being careful to match up the symbols. (+-)



Step 2. Connect lead wire cables to respective channel.



Step 3. Connect lead wire pins to 2 small pads per channel before applying to skin. Remove Pads from film.

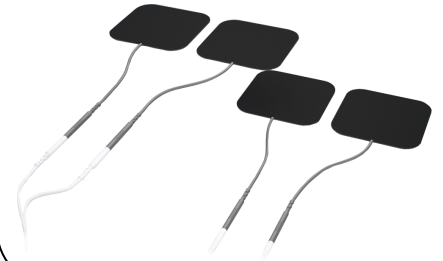

Step 4. Apply Pads: 2 small pads per channel as per placement diagram in manual.



Step 5. Power On: Press ON/+.



Step 6. Treatment Time: Press Mode, then ON/+ or OFF/- to select.



Step 7. Set Therapy Mode: Press Mode. Press ON/+ or OFF/- to select.



Step 9. Set Intensity: Press CH1 or CH2. Press ON/+ or OFF/- to select.



Safety Feature Intensity Level Reset
See steps #2-9 to complete set-up.



WARNINGS & PRECAUTIONS

DO NOT USE THIS SYSTEM IF YOU HAVE A CARDIAC PACEMAKER, IMPLANT DEFIBRILLATOR OR ANY OTHER IMPLANTED METALLIC OR ELECTRONIC DEVICE. DO NOT USE THIS DEVICE FOR UNDIAGNOSED PAIN SYMPTOMS UNTIL CONSULTING A PHYSICIAN. DO NOT USE IF PREGNANT OR IN LABOR. NOT SUITABLE FOR CHILDREN UNDER 16 YEARS OLD. PLEASE REFER TO MANUAL FOR ADDITIONAL WARNING AND PRECAUTIONS.

IMPORTANT: STEPS 1 THRU 4 SHOULD BE PERFORMED WITH THE DEVICE TURNED OFF. ONCE DEVICE IS TURNED ON, DO NOT REMOVE ELECTRODES WITHOUT TURNING OFF THE UNIT.

**This guide is not intended to replace or substitute the ET-1313 manual.*

****Please read the instruction manual completely before using this device.**

For more information, warranty registration and promotions visit us online at www.iReliev.com

